



National Accreditation Board for Testing and Calibration Laboratories

(A Constituent Board of Quality Council of India)



CERTIFICATE OF ACCREDITATION

C I PROFICIENCY TESTING PVT. LTD.

has been assessed and accredited in accordance with the standard

ISO/IEC 17043:2010

"Conformity Assessment - General Requirements for Proficiency Testing"

for its facilities at

H-13 D, Electronic Complex Road No.1, IPIA, Kota, Rajasthan

in the field of

Proficiency Testing Provider

Certificate Number PC-1032

Issue Date 05/11/2018

Valid Until 04/11/2020

This certificate remains valid for the Scope of Accreditation as specified in the annexure subject to continued satisfactory compliance to the above standard & the relevant requirements of NABL.

(To see the scope of accreditation of this Proficiency Testing Provider, you may also visit NABL website www.nabl-india.org)

Signed for and on behalf of NABL



8907697040000000022

Anil Relia

Anil Relia
Chief Executive Officer



National Accreditation Board for Testing and Calibration Laboratories

(A Constituent Board of Quality Council of India)



SCOPE OF ACCREDITATION

PT Provider CI Proficiency Testing Pvt. Ltd., H-13 D Electronic Complex Road No. 1, IPIA, Kota, Rajasthan

Accreditation Standard ISO/IEC 17043:2010

Certificate Number PC-1032 Page 1 of 3

Validity 05.11.2018 to 04.11.2020 Last Amended on --

S.No.	Proficiency Testing Scheme	Proficiency Testing Item	Analyte/ Parameter/ Test Method
-------	----------------------------	--------------------------	---------------------------------

ELECTRO-TECHNICAL CALIBRATION

1.	SEQUENTIAL SCHEME	Decade Resistance Box	DC Resistance
		4½ Digit Multimeter	DC Voltage AC Voltage DC Current AC Current

Anita Rani
Convenor

N. Venkateswaran
Program Manager



National Accreditation Board for Testing and Calibration Laboratories

(A Constituent Board of Quality Council of India)



SCOPE OF ACCREDITATION

PT Provider CI Proficiency Testing Pvt. Ltd., H-13 D Electronic Complex Road No. 1, IPIA, Kota, Rajasthan

Accreditation Standard ISO/IEC 17043:2010

Certificate Number PC-1032 Page 2 of 3


Validity 05.11.2018 to 04.11.2020 Last Amended on --

S.No.	Proficiency Testing Scheme	Proficiency Testing Item	Analyte/ Parameter/ Test Method
-------	----------------------------	--------------------------	---------------------------------

MECHANICAL CALIBRATION

1.	SEQUENTIAL SCHEME	Digital Pressure Gauge	Pressure
----	-------------------	------------------------	----------

-X-X-X-X-X-X-X-X-X-X-

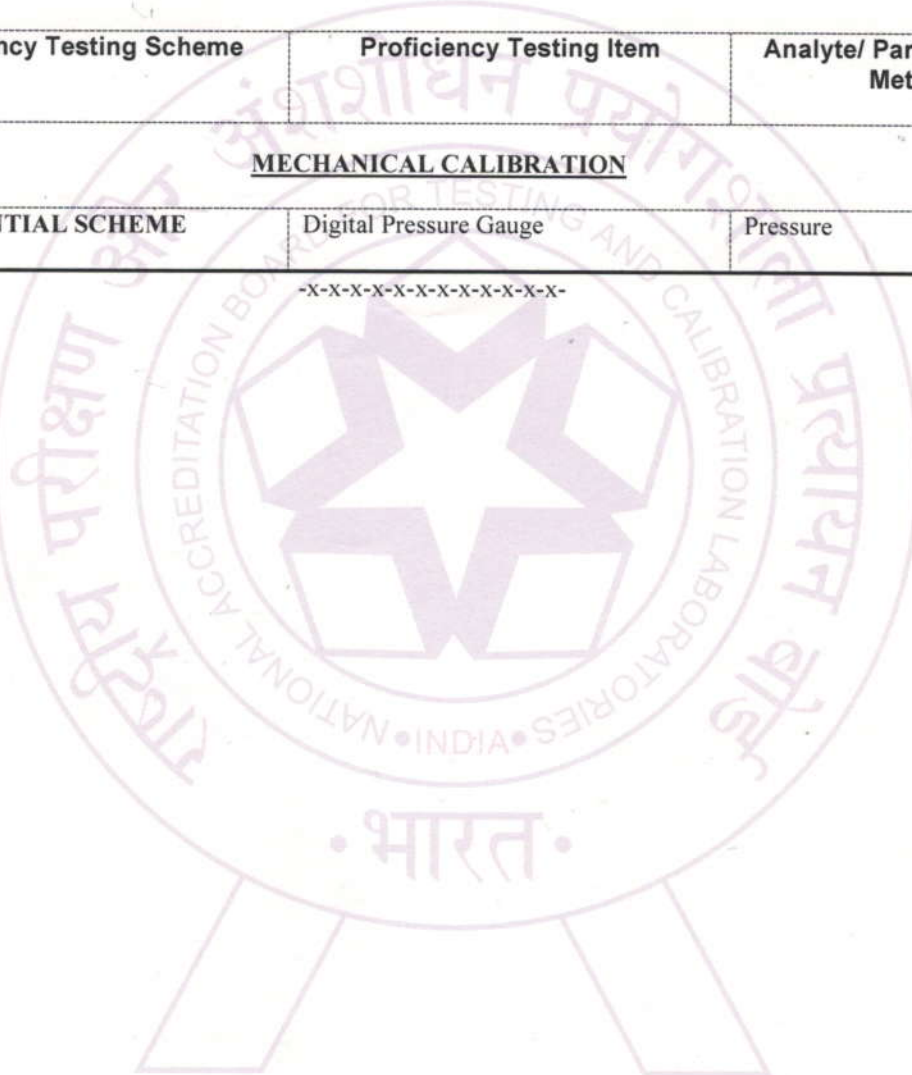

Anita Rani
Convenor

N. Venkateswaran
Program Manager



National Accreditation Board for Testing and Calibration Laboratories

(A Constituent Board of Quality Council of India)



SCOPE OF ACCREDITATION


PT Provider CI Proficiency Testing Pvt. Ltd., H-13 D Electronic Complex Road No. 1, IPIA, Kota, Rajasthan

Accreditation Standard ISO/IEC 17043:2010


Certificate Number PC-1032 Page 3 of 3

Validity 05.11.2018 to 04.11.2020 Last Amended on --

S.No.	Proficiency Testing Scheme	Proficiency Testing Item	Analyte/ Parameter/ Test Method
<u>THERMAL CALIBRATION</u>			
1.	SEQUENTIAL SCHEME	RTD with Indicator	Temperature

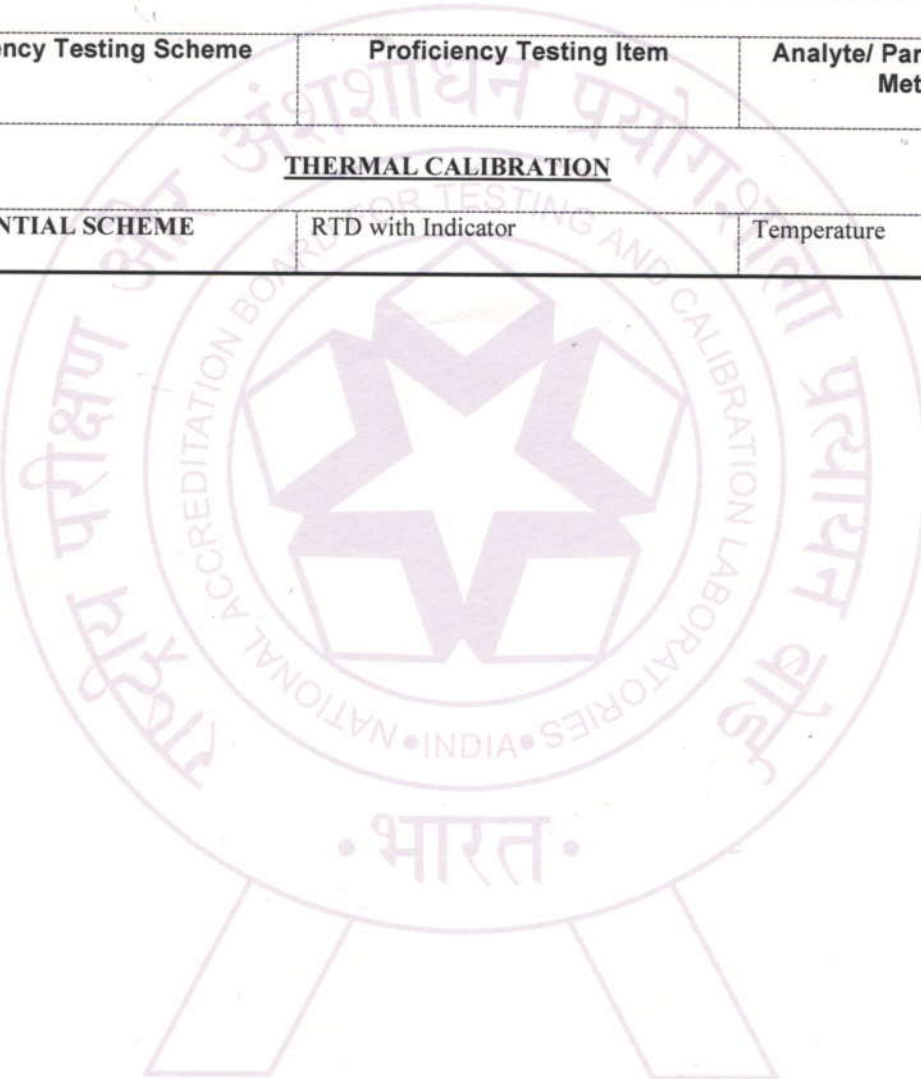


Anita Rani
Convenor


N. Venkateswaran
Program Manager